Verify the validity with the QR code



NB 2163

EU TYPE EXAMINATION CERTIFICATE

Certificate No: 2163-PPE-1306

Respiratory protective devices, filtering half masks to protect against particles manufactured by

İbişler Tekstil Sanayi ve Dış Tic. A.Ş.

Orhan Gazi Mah Tunç Cad. B No:5 B Esenyurt İstanbul TURKEY are tested and evaluated according to

EN 149:2001 + A1:2009 Respiratory Protective Devices -Filtering Half Masks to Protect Against Particles -Requirements, Testing, Marking

Based on the type examination conducted with the evaluation of test reports, technical file according to Personal Protective Equipment Regulation (EU) 2016/425 Annex 5, it is approved that the product meets the requirements of the regulation.

Product Definition

Brand Name: A&Z MED Model: OLI 2025
Filtering half mask
Classification: FFP2 NR

Here by the manufacturer is allowed to use notified body number (2163) and can fix CE mark, as shown below, on the Category III product models given above, with;

- Issuing an appropriate EU Declaration of Conformity according to Personal Protective Equipment Regulation (EU) 2016/425 Annex 9.
- Ongoing successful performance in fulfilment of the requirements set out in Personal Protective Equipment Regulation (EU) 2016/425 and harmonised standards, ensured by assessments based on Annex 7 (Module C2) or Annex 8 (Module D) of the regulation no later than 1 year from the beginning of serial production

This certificate is initially issued on 18/08/2020 and will be valid for 5 years, if there is no change in the relevant harmonised standard affecting the essential health and safety requirements.



Suat KAÇMAZ
UNIVERSAL CERTIFICATION
Director





NB 2163

CERTIFICATE OF CONFORMANCE

Certificate No: 2163-PPE-1306/01

Respiratory protective devices, filtering half masks to protect against particles manufactured by

İBİŞLER TEKSTİL SANAYİ VE DIŞ TİCARET A.Ş.

Orhangazi Mahallesi Tunç Caddesi No:5 34358 Esenyurt ISTANBUL / TURKEY

Continues to fulfil the requirements of

EN 149:2001 + A1:2009 Respiratory Protective Devices -Filtering Half Masks to Protect Against Particles -Requirements, Testing, Marking

Based on the evaluation of test reports and internal quality control audit reports according to EN 149+A1:2009 and Personal Protective Equipment Regulation (EU) 2016/425 Annex VII (Module C2). This certificate implies that the manufactured products show below are in conformance with the approved EU Type Examination model and meets the requirements of the regulation.

Product Definition

	Class	EU Type Examination Certificate		
Model	Class	Serial No	Date	Issuing NB No
A&Z MED / OLI 2025	FFP2 NR	2163-PPE-1306	18.08.2020	2163

Here by the manufacturer is allowed to use notified body number (2163) and can fix CE mark, as shown below, on the Category III product models given above, with;

- Issuing an appropriate EU Declaration of Conformity according to Personal Protective Equipment Regulation (EU) 2016/425 Annex 9.
- Taking all measures necessary so that the manufacturing process and its monitoring
 ensure the homogeneity of production and conformity of the manufactured PPE with
 the type described in the EU type examination certificate.

This certificate is issued on 05/11/2020 and will be valid for one year, until 04/11/2021 if the manufacturer makes no major change in the product designs and manufacturing processes affecting the product performance on the essential health and safety requirement.

CE 2163

Suat KAÇMAZ
UNIVERSAL CERTIFICATION
Director

EU DECLARATION OF CONFORMITY 261-PPE-1306/1

MANUFACTURER

İBİŞLER TEKSTİL SANAYİ VE DIŞ TİCARET ANONİM ŞİRKETİ

Orhangazi Mahallesi Tunç Caddesi No:5 34358 Esenyurt ISTANBUL / TURKEY

Personal Protective Equipment (PPE)

Brand Name: A&Z MED Model: OLI 2025

Particle Filtering Half Mask Classification: FFP2 NR Standard: EN 149:2001+A1:2009

This declaration of conformity is issued under the sole responsibility of the manufacturer above.

The object of the declaration described above is in conformity with the relevant Union harmonization legislation: Personal Protective Equipment Regulation (EU) 2016/425

The Conformity is ensured with the following mechanism:

- Complies with Essential Health and Safety Requirements of Technical harmonized standard EN 149:2001 +A 1:2009
- All required tests referred in above standards are conducted,
- Complies with other relevant harmonized legislation and community standards
- The fulfilment of the relevant health and safety requirements set out in Annex II of (EU) 2016/425 has been demonstrated.

The Notified Body

Universal Certification and Surveillance Service Trade Ltd. Co., Necip Fazıl Bulvarı Keyap Sitesi E2 Blok No: 44/84 Yukarı Dudullu, Ümraniye-Istanbul, Turkey, Notified Body Number 2163 performed the EU type-examination (Module B) and issued the EU type-examination certificate 2163-PPE-1306.

The PPE is subject to the conformity to type assessment procedure based on internal production control plus supervised product checks at random intervals (Module C2), under surveillance of the Notified Body Universal Certification, Notified Body Number 2163.



Olgun İBİŞ

Chief Executive Officer 19.8.2020 İstanbul

IBİŞLER TEKSTİL SAN VE DIŞ TİC A.Ş Orhandazi Mah. Jun Cad Ma:5% BJOK ESON OF ISTANBU

Hangazi Man. July Cap 18.38 Blog 25 Sydy 15 IANSOL di: 0212 602 0405 Fax: 0212 602 04 07 Marman Mururilla VD. 468 052 6462 Tic. Sicil No: 431676

wasis No. 0469052646200026 bilgi@ibisler.com 2163



This is to Certify that



İBİŞLER TEKSTİL SAN. VE DIŞ TİC. A.Ş.

ORHANGAZİ MAH. TUNÇ CAD. NO:5/B ESENYURT / İSTANBUL,TURKEY

Conforms to the Requirements of

ISO 9001:2015

Quality Management System

Tulum ve Medikal Maske Dikimi ve Satışı.

Jumpsuit and Medical Mask Sewing and Sale.

Certificate Number

: Q.020.080.TR

Certification Period

: 3 Years / 16.04.2023

Expiry Date :17.04.2023

Certified Date: 17.04.2020


Approving Officer:









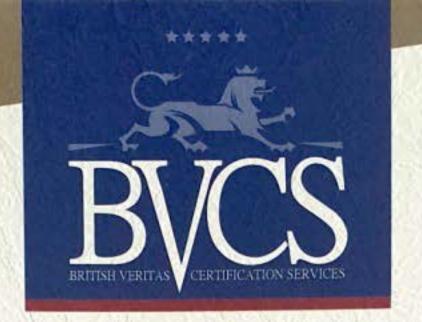

This is to Certify that



İBİŞLER TEKSTİL SAN. VE DIŞ TİC. A.Ş.

ORHANGAZİ MAH. TUNÇ CAD. NO:5/B ESENYURT / İSTANBUL,TURKEY

Conforms to the Requirements of

ISO 13485:2016

Medical Device Quality Management System

Tulum, Medikal Önlük ve Medikal Maske Dikimi ve Satışı.

Jumpsuit, Medical Gowns and Medical Mask Sewing and Sale.

Certificate Number

: M.020.080.TR


Certification Period

: 3 Years / 16.04.2023

Expiry Date : 17.04.2023

Certified Date: 17.04.2020

Approving Officer:







Article 7.17	Clogging: This test is not applied to Particle Filtering Half Mask which is not reusable. (For single shift use devices, the clogging test is optional test. For re-usable devices test is mandatory.)
Article 7.18	Demountable Parts: There are no demountable parts on the product.
Article 8	Testing: All tests conducted according to Clause 8 of this standard is available in the test report and are evaluated in this report for qualification and classification of the mask.
	Marking – Packaging: Necessary markings are available on the product package (box). The manufacturer and its trademark is clearly visible. The type of the mask and the classification including the status of re-usability, the reference to EN 149:2001+A1:2009 standard, the end date of shelf life, using and storage instructions and pictograms and CE mark are available on the product package. The above evaluation is based on the technical document for packaging and marking, for box design. Verified on the technical file.
Article 9	The technical documentation for mask design (drawing) also evaluated for marking requirements, drawing OLI 2025. The mask template (drawing) indicates that the mask will carry information about the manufacturer type of mask, the reference to EN 149+A1:2009 standard and classification including the re-usability of the mask. The manufacturer also printed CE mark with our Notified Body number. The mask do not have sub-assemblies. The marking statement given in the technical documentation was not available on the tested specimen, the manufacturer shall consider to use the marking as stated in the technical file in case of serial manufacturing. Model OLI 2025 drawing exists in the technical file of the manufacturer.
Article 10	Information to be supplied by the manufacturer: In each of the smallest commercially available packaging of the product, implementation (installation instructions) pre-use controls, warning and usage limitations, storage and meanings of symbols / pictograms are defined. User instruction document in the technical file found to be appropriate. The manufacturer shall include this documented user information text in every smallest commertially available package.

PREPARED BY	APPROVED BY
Osman CAMCI PPE Expert	Suat KAÇMAZ General Manager



UNIVERSAL CERTIFICATION and SURVEILLANCE SERVICES TRADE CO.

Necip Fazil Bulvari Keyap Sitesi E2 Blok No:44/84 Yukari Dudullu Umraniye, Istanbul / TURKEY

TEST REPORT

Report Date: 17.08.2020

Report Number: 08-2020-T-0309

CLIENT and SAMPLE INFORMATION

TEST OWNER	İBİŞLER TEKSTİL SANAYİ VE DIŞ TİC. A.Ş.					
ADDRESS	ORHAN GAZİ MAH TUNÇ CAD. B NO:5 B ESENYURT İSTANBUL					
SAMPLE DESCRIPTION	Folding type p	protective ma	sk			
BRAND NAME – MODEL	A&Z MED / C	DLI 2025				
TESTING STANDARD	EN 149+A1:2	009				
CASE NUMBER	CE-PPE-3315					
SAMPLE RECEIVE DATE	20.07.2020 TESTING START DATE 20.07.2020					
DISINFECTION INSTRUCTION If applicable	Not given, sin	gle use only				
NUMBER OF SAMPLES	50	SAMPLE I	Ds:	1 – 46		
AS RECEIVED SAMPLE NO	26-46					
	Simulated wearing treatment 1-2-3-4-5-6-7-8-9 (As Received)				eceived)	
CONDITIONING SAMPLE NO	Temperature conditioning Strength) 10-11-12-13-14-15 (Sample after test of Mechanic			ple after test of Mechanical		
			16-17-18-19-20-21-22-23-24-25 (As Received)			
	Mechanical st	rength	10-	11-12-13-14-15 (As R	eceived).	

The results given in this test report belongs to the samples tested. The report content cannot be recreated partially without the written consent of UNIVERSAL CERTIFICATION.

UNIVERSAL SERTIFIKASYON VE GÖZETİM HİZM. TİC. LTD. ŞTI. 11 BUVAT, Keyab Sitesi, E2 Blok, No:44/84 İkarı Dudully-Umraniye/ISTAN BUN. no: 0216/455 80 80 Faks: 0216 455 80 08 Sarigazi V.D. 892 025 8722

Suat KAÇMAZ
Director



1. REPORT SUMMARY

TEST STANDARD	TEST NAME	RESULT	EVALUATION	
EN 149:2001 +				
A1:2009 clause 8.5	Total Inward Leakage Testing	Pass	FFP2	
EN 13274-1:2001	100			
EN 149:2001 +				
A1:2009 clause 8.11	Penetration of Filter Material	Pass	FFP2	
EN 13274-7:2019				
EN 149:2001 +				
A1:2009 clause 8.6	Flammability Testing	Pass	See results	
EN 13274-4:2001				
EN 149:2001 +	Carbon Dioxide Content of The Inhalation			
A1:2009 clause 8.7		Pass	See results	
EN 13274-6:2001	Air Testing			
EN 149:2001 +	Breathing Inhalation Resistance-30 l/min	Pass	See results	
A1:2009 clause 8.9		1 455	See resures	
EN 13274-3:2001	Breathing Inhalation Resistance-95 l/min	Pass	See results	
EN 149:2001 +				
A1:2009 clause 8.9	Exhalation Resistance, flow rate 160 l/min	Pass	See results	
EN 13274-3:2001				





7.4 PACKAGING (EN 149:2001 + A1:2009 clause 8.2)

Test Method: Clause 8.2-Visual inspection

REQUIREMENT	RESULTS	COMMENT
Particle filtering half masks shall be offered for sale packaged in such a way that they are protected against mechanical damage and contamination before use.	Pass	The masks were packaged in sealed plastic bags, in larger plastic bags inside a large cardboard box that gave some protection against mechanical damage or contamination before use

Lab A

7.5 MATERIAL (EN 149:2001 + A1:2009 clause 8.2, 8.3.1, 8.3.2)

Test Method: Clause 8.2-Visual inspection

Clause 8.3.1-Simulated wearing treatment

A breathing machine is adjusted to 25 cycles/min and 2,0 l/stroke. The particle filtering half mask was mounted on a Sheffield dummy head.

For testing, a saturator is incorporated in the exhalation line between the breathing machine and the dummy head, the saturator being set at a temperature in excess of 37 °C to allow for the cooling of the air before it reaches the mouth of the dummy head.

The air has been saturated at (37 ± 2) °C at the mouth of the dummy head

Clause 8.3.2-Temperature conditioning

The ambient temperature for testing has been between 16 °C and 32 °C and the temperature limits has been subject to an accuracy of ± 1 °C.

- a) for 24 h to a dry atmosphere of (70 ± 3) °C;
- b) for 24 h to a temperature of (-30 ± 3) °C; and allow to return to room temperature for at least 4 h between exposures and prior to subsequent testing. The conditioning has been carried out in a manner which ensures that no thermal shock occurs.

REQUIREMENT	RESULTS	<u>COMMENT</u>
Materials used shall be suitable to withstand handling and wear over the period for which the particle filtering half mask is designed to be used.	Pass	The materials used were able to withstand handling and wear during the limited laboratory testing carried out.
Any material from the filter media released by the air flow through the filter shall not constitute a hazard or nuisance for the wearer.	Pass	It was not constitute a hazard or nuisance for the wearer.
After undergoing the conditioning described in 8.3.1 none of the particle filtering half masks shall have suffered mechanical failure of the facepiece or straps.	Pass	None of the specimens conditioned suffered mechanical failure.
When conditioned in accordance with 8.3.1 and 8.3.2 the particle filtering half mask shall not collapse.	Pass	None of the specimens had not collapse after conditioning.

Lab B





7.6 CLEANING AND DISINFECTING (EN 14922001 HFA1152009 Elause 8.4, 8.5, 8.11)

Test Method: Described in Clause 8.4, 8.5 and 8.11

REQUIREMENT	RESULTS	COMMENT
If the particle filtering half mask is designed to be re-usable, the materials used shall withstand the cleaning and disinfecting agents and procedures to be specified by the manufacturer. With reference to 7.9.2, after cleaning and disinfecting the re-usable particle filtering half mask shall satisfy the penetration requirement of the relevant class.	N/A	This article is not applicable for tested protective mask which is single use disposable mask.

7.7 PRACTICAL PERFORMANCE (EN 149:2001 + A1:2009 clause 8.4)

Test Method: Described in Clause 8.4

REQUIREMENT	RESULTS	COMMENT
The particle filtering half mask shall undergo practical performance tests under realistic conditions. These general tests serve the purpose of checking the equipment for imperfections that can not be determined by the tests described elsewhere in this standard.	No imperfections	Detail refer to Annex I
Two as received mask samples are used by two subject for the walking (10 mins walking with a speed of 6km/h) and work simulation (bended walking, crawling and basket filling exercises) tests.	=	

Annex I-Test Result:

Number of sample: 29 (A.R), 30 (A.R)

Assessed elements	Positive Assessment	Negative Assessment	Requirements in accordance with EN 149:2001+A1:2009	Assessment of Test Result Conformity / Nonconformity
The face piece fitting Head harness comfort Security of fastenings Field of vision	2 2 2 2 2	0 0 0 0	Filtering half masks should not have imperfections related to wearer's acceptance	Filtering half masks fulfil requirements of the standard EN 149:2001 + A1:2009 given in 7.7 No imperfections

The subjects (MEG and MA) were able to complete the exercises and did not report any nuisance or problem with the mask. Lab B

7.8 FINISH OF PARTS (EN 149:2001 + A1:2009 clause 8.2)

Test Method: Described in Clause 8.2

REQUIREMENT	RESULTS	COMMENT
Parts of the device likely to come into contact with the wearer shall have no sharp edges or burrs.	Pass	None of the specimens used in laboratory testing showed evidence of sharp edges or burrs while visual inspection and performance tests.

Lab A

UNIVERSAL SERTIFIKASYON VE GÖZETİM HİZM. TİC. LTD. ŞTİ. Necip Fazil Bulvarı, Keyap Sitesi, E2 Blok, No:44/84 Yukarı Dudullu-Ümraniye/ISTANBUL Telefon: 0216 455 80 80 Faks: 0216 455 80 08 Sarigazi V.D. 892 025 8722



7.9.1 TOTAL INWARD LEAKAGE (EN 149:2000 R-TA 1::2009\chanse 8:5)

Test Method: Described in Clause 8.5

REQUIREMENT	RESULTS	COMMENT
The total inward leakage consists of three components: face seal leakage, exhalation value leakage (if exhalation value fitted) and filter penetration. For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual results shall be not greater than: 25 % for FFP1, 11 % for FFP2, 5 % for FFP3 and in addition at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall not be greater than: 22 % for FFP1, 8 % for FFP2, 2 % for FFP3	Pass	Classified as FFP2 Detail refer to Annex II

Annex II-Test Result:

The test results obtained are given in the tables as follows

Test Subject	No of sample	Cond.	1. Walk (%)	Head side/ side (%)	Head up/down (%)	Talk (%)	2. Walk (%)	Average (%)
1	31	A.R.	5,37	5,93	5,15	6,40	6,03	5,78
2	32	A.R.	4,58	4,76	5,92	5,98	4,60	5,17
3	33	A.R.	6,00	6,20	4,60	4,72	4,67	5,24
4	34	A.R.	4,84	5,88	6,02	5,59	5,53	5,57
5	35	A.R.	4,91	6,23	5,27	6,27	5,67	5,67
6	16	T.C.	4,87	4,75	5,71	5,25	6,37	5,39
7	17	T.C.	6,51	5,32	4,90	6,48	5,71	5,78
8	18	T.C.	5,43	6,26	5,26	6,08	5,38	5,68
9	19	T.C.	6,34	5,10	6,30	5,94	6,30	5,99
10	20	T.C.	6,17	5,42	5,87	5,91	6,06	5,89
All 50 individual exercise results were not greater than 11 % All 10 individual wearer arithmetic means were not greater than 8 %.						Pass (FFP2)		

Test Subject	Face Length (mm)	Face Width (mm)	Face Depth (mm)	Mouth Width (mm)
1	117	155	130	60
2	113	148	128	62
3	112	160	134	59
4	115	148	125	61
5	120	158	132	57
6	118	150	134	59
7	115	152	130	57
8	117	155	134	59
9	114	149	128	57
10	110	150	131	55

For Information Only

Lab B





7.9.2 PENETRATION OF FILTER MATERIAE (EN11#9:2001T+1A1 12009 clause 8.11)

Test Method: Described in Clause 8.11

REQUIREMENT			RESULTS	COMMENT	
Classification	NaCl test 95 l/min %max	Paraffin oil test 95 l/min %max	Pass	Detail refer to Annex IIIA and IIIB	
FFP1 FFP2 FFP3	20 6 1	20 6 1			

Annex IIIA-Test Result:

The test results obtained are given in the tables as follows:

No. of Sample	Condition	Penetration of Sodium Chloride in accordance with EN 13274- 7:2019 [%] Flow rate 95 l/min	Requirements in accordance with EN 149:2001+A1:2009	Assessment of Test Result Conformity / Nonconformity
36		0,83		Passed
37	As received	0,87		
38		0,66	FFP1 < 20 %	Filtering half masks
1	Cimulated wagning	0,70	1111 = 20 70	fulfil the requirements of
2	Simulated wearing treatment	1,09	FFP2 ≤ 6 %	the standard EN
3	treatment	0,72	1112 = 0.70	149:2001+A1:2009
10	Mechanical strength +	0,50	FFP3 < 1 %	given in 7.9.2 in range of
11	Temperature	0,78	naan = 118	the first, second
12	conditioned	1,09		protection class (FFP1, FFP2)

Annex IIIB-Test Result:

The test results obtained are given in the tables as follows;

No. of Sample	Condition	Penetration of Paraffin Oil Mist in accordance with EN 13274-7:2019 [%] Flow rate 95 l/min	Requirements in accordance with EN 149:2001+A1:2009	Assessment of Test Result Conformity / Nonconformity
39		1,62		Passed
40	As received	1,14		
41		1,96	FFP1 ≤ 20 %	Filtering half masks fulfil
4	6: 1.1.1	1,70		the requirements of the
5	Simulated wearing	1,65	FFP2 ≤ 6 %	standard EN
6	treatment	1,61		149:2001+A1:2009 given
13	Mechanical strength +	1,66	FFP3 ≤ 1 %	in 7.9.2 in range of the first,
14	Temperature	1,39		second protection classes
15	conditioned	1,98		(FFP1, FFP2)

Lab A + B





7.10 COMPATIBILITY WITH SKIN (EN 149:2001 7-141:2009 Tlause8.4, 8.5)

Test Method: Described in Clause 8.4 and 8.5.

REQUIREMENT	RESULTS	COMMENT
Materials that may come into contact with the wearer's skin shall not be known to be likely to cause irritation or any other adverse effect to health.	Pass	No irritation or any other adverse effect to health or sensitivity reported by the subjects during the practical performance and TIL tests.

Lab B

7.11 FLAMMABILITY (EN 149:2001 + A1:2009 clause 8.6)

Test Method: Described in Clause 8.6

<u>REQUIREMENT</u>	RESULTS	COMMENT
The material used shall not present a danger for the wearer and shall not be of highly flammable nature. When tested, the particle filtering half mask shall not burn or not to continue to burn 5s after removal from the flame.	Pass	Detail refer to Annex IV

Annex IV-Test Result: The test results obtained are given in the tables as follows:

No. of Sample	Condition	Visual inspection	Requirements in accordance with EN 149:2001+A1:2009	Assessment of Test Result Conformity / Nonconformity
45		0,3 s	Filtering half mask	Passed
46	As received	0,3 s	shall not burn or not	Filtering half masks fulfil
21	Temperature	0,5 s	continue to burn for more than 5 s after	requirements of the standard EN 149:2001 +
22	conditioned	0,4 s	removal from the flame	A1:2009 given in 7.11

Lab B

7.12 CARBON DIOXIDE CONTENT OF THE INHALATION AIR (EN 149:2001 + A1:2009 clause 8.7)

Test Method: Described in Clause 8.7

REQUIREMENT	RESULTS	COMMENT	
The carbon dioxide content of the inhalation air (dead space) shall not exceed an average of 1,0 % (by volume)	Pass	Detail refer to Annex V	

Annex V-Test Result: The test results obtained are given in the tables as follows:

No. of Sample	Condition	CO ₂ content of the inhalation air [%] by volume	An average CO ₂ content of the inhalation air [%] by volume	Requirements in accordance with EN 149:2001+A1:2009	Assessment of Test Result Conformity / Nonconformity
26		0,64		CO ₂ content of the inhalation air shall	Passed Filtering half masks fulfil
27	As received	0,75	0,71	not exceed an	requirements of the
28		0,74	9	average of 1,0% by volume	standard EN 149:2001 + A1:2009 given in 7.12

Lab B

UNIVERSAL SERTIFIKASYON VE GÖZETİM HİZM.

VE GOZETIM HIZM.

TIC. LTD. \$TI.

Ip Fazil Bulvari, Keyap Sitesi, EZ Blok, No:44/84

Yukari Dudullu-Umraniye/ISTANBUL

qefon: 0216 455 80 80 Faks: 0216 455 80 08

Sarigazi V.D. 892 025 8722

Page 7 / 11



7.13 HEAD HARNESS (EN 149:2001 + A1:2009 clause 8.4, 8.5)

Test Method: Described in Clause 8.4, 8.5

REQUIREMENT	RESULTS	COMMENT
The head harness shall be designed so that the particle filtering half-mask can be donned and removed easily.	Pass	No problem with the head harness reported by the wearers during the practical performance test.
The head harness shall be adjustable or self-adjusting and shall be sufficiently robust to hold the particle filtering half mask firmly in position and capable of maintaining total inward leakage requirements for the device.	Pass	No problem with the head harness reported by the wearers during the practical performance test.

7.14 FIELD OF VISION (EN 149:2001 + A1:2009 clause 8.4)

Test Method: Described in Clause 8.4

REQUIREMENT	RESULTS	COMMENT
The field of vision is acceptable if determined so in practical performance tests.	Pass	There were no adverse comments following practical performance tests.

Lab B

7.15 EXHALATION VALVE (EN 149:2001 + A1:2009 clause 8.2, 8.3.4, 8.8, 8.9.1)

Test Method: Clause 8.2, 8.3.4, 8.8, 8.9.1

REQUIREMENT	RESULTS	COMMENT
A particle filtering half mask may have one or more exhalation valve(s), which shall function correctly in all orientations.	N/A	No exhalation valve in tested samples.
If an exhalation valve is provided it shall be protected against or be resistant to dirt and mechanical damage and may be shrouded or may include any other device that may be necessary for the particle filtering half mask to comply with 7.9	N/A	No exhalation valve in tested samples.
Exhalation valve(s), if fitted, shall continue to operate correctly after a continuous exhalation flow of 300 l/min over a period of 30s.	N/A	No exhalation valve in tested samples.
When the exhalation valve housing is attached to the face blank, it shall withstand axially a tensile force of 10N applied for 10s.	N/A	No exhalation valve in tested samples.

Lab -





7.17 CLOGGING (EN 149:2001 + A1:2009 clause 8.9, 8H0)C ATION

Test Method: Described in Clause 8.8, 8.10

REQUIREMENT	RESULTS	COMMENT
Valved particle filtering half masks: After clogging the inhalation resistances shall not exceed: FFP1:4mbar, FFP2:5mbar, FFP3:7mbar at 95L/min continuous flow. The exhalation resistance shall not exceed 3mbar at 160L/min continuous flow. Valveless particle filtering half masks: After clogging the inhalation resistances shall not exceed: FFP1:3mbar, FFP2:4mbar, FFP3:5mbar at	NAs	This is optional test and not desired by client.
95L/min continuous flow	200	

Lab -

7.18 DEMOUNTABLE PARTS (EN 149:2001 + A1:2009 clause 8.2)

Test Method: Described in Clause 8.2

REQUIREMENT	RESULTS	COMMENT	
All demountable parts (if fitted) shall be readily connected and secured, where possible by hand	N/A	No demountable part.	

Lab -

Pass	Requirement satisfied.	
NCR	Requirement not satisfied. Refer to the "Result details" section for more information.	
NAs	Assessment not carried out.	
N/A	Requirement not applicable.	

LABORATORY INFORMATION

Code	Laboratory Name	Competency Explanations	
Lab A	UNIVERSAL SERTIFIKASYON VE GOZETIM HIZMETLERI TIC. LTD. STI.	Internal Laboratory Services of Notified Body	
Lab B	GCNTR ULUSLARARASI BELGELENDIRME, GOZETIM, EGITIM VE DIS TICARET LIMITED SIRKETI KOCAELI DILOVA SUBESI	Laboratory holds an accreditation by Turkish Accreditation Agency with number AB-1252-T according to EN ISO/IEC 17025:2017.	
•	of the laboratories is also under supervision / assessment of UNIVERSAL CERTIFICATION based on the provisions of EN ISO/IEC 17065 Requirements for bodies certifying products, processes and services standard.		
•	Each test result given in this test report shown with the issuing laboratory code.		

UNIVERSAL SERTIFIKASYON VE GOZETIM HIZM. TIC. LTD. STI.

Necip Fazil Bulvarı, Keyap Sitesi, Ez Blok, No:44/84

Lukarı Dudullu-Umraniye/STANBUL

Afon: 0216 455 80 80 Fasi: 0216 455 80 08

Sarıgazi V.D. 892 025 8722





- End of Report -

